

SPEC SHEET

Plug-in Type Digital Indicating Conductivity Meter

WIL-102- ECL (Low Concentration)

- DIN rail mounted type
- Various settings, calibration operable via software communication (RS-485)
- 24 V power supply available (user-specified)
- Transmission output 1 and 2 (optional)



Name	Plug-in type digital indicating conductivity meter																																																															
Model	<table><tr><td>W I L - 1 0</td><td>2</td><td>-EC</td><td></td><td></td><td>, <table><tr><td></td><td></td><td></td><td></td></tr></table></td><td></td></tr><tr><td>Input points</td><td>2</td><td></td><td></td><td></td><td></td><td>2 points</td></tr><tr><td rowspan="2">Input</td><td rowspan="2">EC</td><td rowspan="2"></td><td rowspan="2"></td><td rowspan="2"></td><td rowspan="2"></td><td>2-electrode conductivity sensor (Temperature element: Pt100) (*1)</td></tr><tr><td>2-electrode conductivity sensor (Temperature element: Pt1000) (*1)</td></tr><tr><td colspan="2">Concentration</td><td>L</td><td></td><td></td><td></td><td>Low concentration</td></tr><tr><td colspan="2" rowspan="2">Power supply voltage</td><td rowspan="2">1</td><td></td><td></td><td></td><td>100 to 240 V AC (standard)</td></tr><tr><td></td><td></td><td></td><td>24 V AC/DC (*2)</td></tr><tr><td colspan="4" rowspan="3">Option</td><td>EVT</td><td></td><td>2-points Contact output</td></tr><tr><td>TA</td><td></td><td>1-point Transmission output 1-point Contact output</td></tr><tr><td>TA2</td><td></td><td>2-points Transmission output</td></tr></table> (*1) This input temperature specification was specified at the time of ordering. (*2) Supply voltage 100 to 240 V AC is standard. When ordering 24 V AC/DC, enter 1 in Power supply voltage, after 'ECL'. Accessories sold separately: Socket: ASK-001-1 (Finger-safe, Ring terminals unusable)							W I L - 1 0	2	-EC			, <table><tr><td></td><td></td><td></td><td></td></tr></table>						Input points	2					2 points	Input	EC					2-electrode conductivity sensor (Temperature element: Pt100) (*1)	2-electrode conductivity sensor (Temperature element: Pt1000) (*1)	Concentration		L				Low concentration	Power supply voltage		1				100 to 240 V AC (standard)				24 V AC/DC (*2)	Option				EVT		2-points Contact output	TA		1-point Transmission output 1-point Contact output	TA2		2-points Transmission output
W I L - 1 0	2	-EC			, <table><tr><td></td><td></td><td></td><td></td></tr></table>																																																											
Input points	2					2 points																																																										
Input	EC					2-electrode conductivity sensor (Temperature element: Pt100) (*1)																																																										
						2-electrode conductivity sensor (Temperature element: Pt1000) (*1)																																																										
Concentration		L				Low concentration																																																										
Power supply voltage		1				100 to 240 V AC (standard)																																																										
						24 V AC/DC (*2)																																																										
Option				EVT		2-points Contact output																																																										
				TA		1-point Transmission output 1-point Contact output																																																										
				TA2		2-points Transmission output																																																										
Measurement range (Rated scale)	<table><tr><th>Input</th><th>Cell constant</th><th>Scale Range</th><th>Resolution</th></tr><tr><td rowspan="22">Conductivity</td><td rowspan="10">Cell constant 0.01/cm</td><td>0.000 to 2.000 $\mu\text{S/cm}$</td><td>0.001 $\mu\text{S/cm}$</td></tr><tr><td>0.00 to 20.00 $\mu\text{S/cm}$</td><td>0.01 $\mu\text{S/cm}$</td></tr><tr><td>0.00 to 50.00 $\mu\text{S/cm}$</td><td>0.01 $\mu\text{S/cm}$</td></tr><tr><td>0.000 to 0.200 mS/m</td><td>0.001 mS/m</td></tr><tr><td>0.000 to 2.000 mS/m</td><td>0.001 mS/m</td></tr><tr><td>0.000 to 5.000 mS/m</td><td>0.001 mS/m</td></tr><tr><td>0.00 to 2.00 mg/L</td><td>0.01 mg/L</td></tr><tr><td>0.0 to 20.0 mg/L</td><td>0.1 mg/L</td></tr><tr><td>0.0 to 50.0 mg/L</td><td>0.1 mg/L</td></tr><tr><td rowspan="10">Cell constant 0.1/cm</td><td>0.00 to 20.00 $\mu\text{S/cm}$</td><td>0.01 $\mu\text{S/cm}$</td></tr><tr><td>0.00 to 50.00 $\mu\text{S/cm}$</td><td>0.01 $\mu\text{S/cm}$</td></tr><tr><td>0.0 to 500.0 $\mu\text{S/cm}$</td><td>0.1 $\mu\text{S/cm}$</td></tr><tr><td>0.000 to 2.000 mS/m</td><td>0.001 mS/m</td></tr><tr><td>0.000 to 5.000 mS/m</td><td>0.001 mS/m</td></tr><tr><td>0.00 to 50.00 mS/m</td><td>0.01 mS/m</td></tr><tr><td>0.0 to 20.0 mg/L</td><td>0.1 mg/L</td></tr><tr><td>0 to 200 mg/L</td><td>1 mg/L</td></tr><tr><td>0 to 500 mg/L</td><td>1 mg/L</td></tr><tr><td rowspan="3">Cell constant 1.0/cm</td><td>0.0 to 200.0 $\mu\text{S/cm}$</td><td>0.1 $\mu\text{S/cm}$</td></tr><tr><td>0.00 to 20.00 mS/m</td><td>0.01 mS/m</td></tr><tr><td>0 to 200 mg/L</td><td>1 mg/L</td></tr><tr><td>Temperature (Pt100 or Pt1000)</td><td></td><td>0.0 to 100.0°C</td><td>0.1°C</td></tr></table> Decimal point place is selectable for temperature indication.							Input	Cell constant	Scale Range	Resolution	Conductivity	Cell constant 0.01/cm	0.000 to 2.000 $\mu\text{S/cm}$	0.001 $\mu\text{S/cm}$	0.00 to 20.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$	0.00 to 50.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$	0.000 to 0.200 mS/m	0.001 mS/m	0.000 to 2.000 mS/m	0.001 mS/m	0.000 to 5.000 mS/m	0.001 mS/m	0.00 to 2.00 mg/L	0.01 mg/L	0.0 to 20.0 mg/L	0.1 mg/L	0.0 to 50.0 mg/L	0.1 mg/L	Cell constant 0.1/cm	0.00 to 20.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$	0.00 to 50.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$	0.0 to 500.0 $\mu\text{S/cm}$	0.1 $\mu\text{S/cm}$	0.000 to 2.000 mS/m	0.001 mS/m	0.000 to 5.000 mS/m	0.001 mS/m	0.00 to 50.00 mS/m	0.01 mS/m	0.0 to 20.0 mg/L	0.1 mg/L	0 to 200 mg/L	1 mg/L	0 to 500 mg/L	1 mg/L	Cell constant 1.0/cm	0.0 to 200.0 $\mu\text{S/cm}$	0.1 $\mu\text{S/cm}$	0.00 to 20.00 mS/m	0.01 mS/m	0 to 200 mg/L	1 mg/L	Temperature (Pt100 or Pt1000)		0.0 to 100.0°C	0.1°C			
Input	Cell constant	Scale Range	Resolution																																																													
Conductivity	Cell constant 0.01/cm	0.000 to 2.000 $\mu\text{S/cm}$	0.001 $\mu\text{S/cm}$																																																													
		0.00 to 20.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$																																																													
		0.00 to 50.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$																																																													
		0.000 to 0.200 mS/m	0.001 mS/m																																																													
		0.000 to 2.000 mS/m	0.001 mS/m																																																													
		0.000 to 5.000 mS/m	0.001 mS/m																																																													
		0.00 to 2.00 mg/L	0.01 mg/L																																																													
		0.0 to 20.0 mg/L	0.1 mg/L																																																													
		0.0 to 50.0 mg/L	0.1 mg/L																																																													
		Cell constant 0.1/cm	0.00 to 20.00 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$																																																												
	0.00 to 50.00 $\mu\text{S/cm}$		0.01 $\mu\text{S/cm}$																																																													
	0.0 to 500.0 $\mu\text{S/cm}$		0.1 $\mu\text{S/cm}$																																																													
	0.000 to 2.000 mS/m		0.001 mS/m																																																													
	0.000 to 5.000 mS/m		0.001 mS/m																																																													
	0.00 to 50.00 mS/m		0.01 mS/m																																																													
	0.0 to 20.0 mg/L		0.1 mg/L																																																													
	0 to 200 mg/L		1 mg/L																																																													
	0 to 500 mg/L		1 mg/L																																																													
	Cell constant 1.0/cm		0.0 to 200.0 $\mu\text{S/cm}$	0.1 $\mu\text{S/cm}$																																																												
		0.00 to 20.00 mS/m	0.01 mS/m																																																													
		0 to 200 mg/L	1 mg/L																																																													
	Temperature (Pt100 or Pt1000)		0.0 to 100.0°C	0.1°C																																																												

(*1) This input temperature specification was specified at the time of ordering.

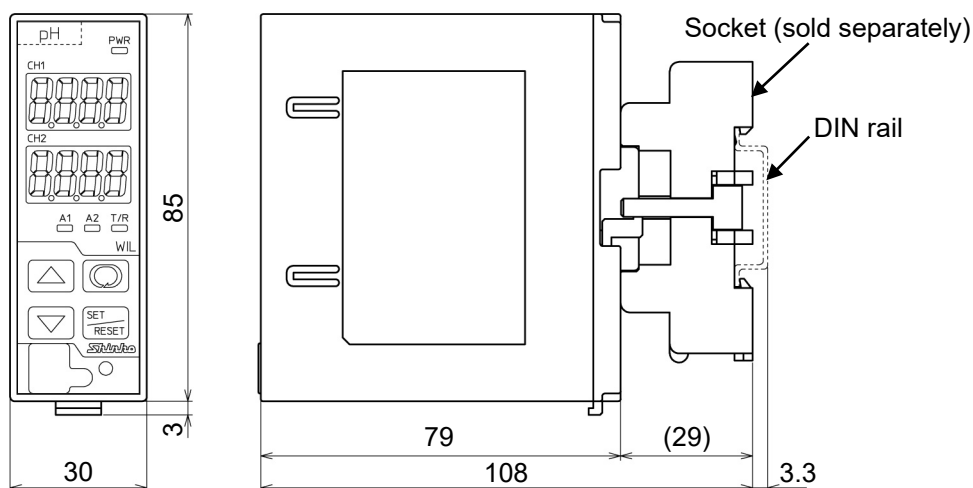
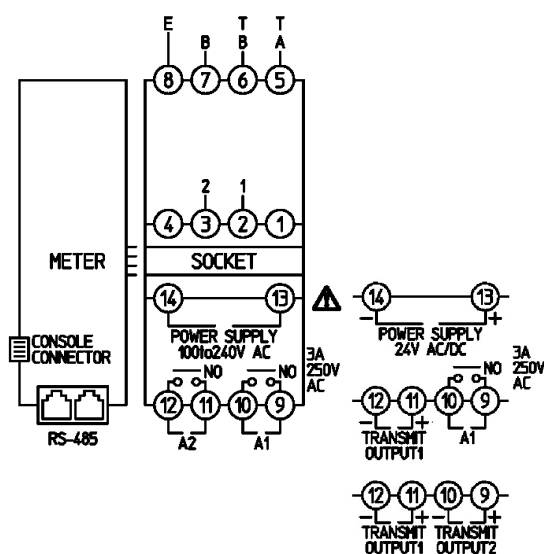
(*2) Supply voltage 100 to 240 V AC is standard.

When ordering 24 V AC/DC, enter 1 in Power supply voltage, after 'ECL'.

Accessories sold separately: Socket: ASK-001-1 (Finger-safe, Ring terminals unusable)

Repeatability	Conductivity: $\pm 0.5\%$ of input span TDS conversion: $\pm 1.5\%$ of input span
Linearity	Conductivity: $\pm 0.5\%$ of input span TDS conversion: $\pm 1.5\%$ of input span
Indication accuracy	Temperature: $\pm 1^{\circ}\text{C}$
Conductivity adjustment	Conductivity Zero adjustment: Zero adjustment value range: -10% of input span to 10% of input span Conductivity Span adjustment: Span adjustment value range: 0.700 to 1.300
Temperature adjustment	Adjustment range: -10.0 to 10.0 $^{\circ}\text{C}$
TDS conversion function	For Conductivity SI unit (mS/m): $\text{TDS}(\text{mg/L}) = \text{L}(\text{mS/m}) \times \text{K} \times 10$ For Conductivity older unit ($\mu\text{S/cm}$): $\text{TDS}(\text{mg/L}) = \text{L}(\mu\text{S/cm}) \times \text{K}$ K: TDS conversion factor, L: Conductivity
Self-diagnosis	The CPU is monitored by a watchdog timer, and if an abnormal status occurs, the instrument is switched to warm-up status.
Temperature compensation element	2-electrode conductivity sensor (Temperature element: Pt100) 2-electrode conductivity sensor (Temperature element: Pt1000)
Temperature compensation range	0.0 to 100.0 $^{\circ}\text{C}$
Ambient temperature	0 to 50 $^{\circ}\text{C}$ (32 to 122 $^{\circ}\text{F}$)
Ambient humidity	35 to 85 %RH (Non-condensing)
Power supply (user-specified)	WIL-102-ECL: 100 to 240 V AC 50/60 Hz Allowable fluctuation range: 85 to 264 V AC WIL-102-ECL 1: 24 V AC/DC 50/60 Hz Allowable fluctuation range: 20 to 28 V AC/DC
Structure	DIN rail mounted Case: Flame-resistant resin, Color: Light gray Front panel: Membrane sheet
Protection structure	Overvoltage category II, Pollution degree 2 (IEC61010-1)
Safety standards	RoHS directive compliant
Dimensions	W30 x H88 x D108 mm (including socket)
Weight	Approx. 200 g (including socket)
Contact output (EVT option)	Relay contact 1a (Bit reading via 2 status flags for 1 output in Serial communication) 2-points Contact output Control capacity: 3 A 250 V AC (Resistive load), 1 A 250 V AC (Inductive load, $\cos\phi=0.4$), Electrical life: 100,000 cycles, Control action: ON/OFF control
Transmission output 1 (TA option)	Converting pH or temperature to analog signal every input sampling period, outputs the value in current. (Factory default: Conductivity) If Transmission output 1 high limit and low limit are set to the same value, Transmission output 1 will be fixed at 4 mA DC. Resolution: 12000 Current: 4 to 20 mA DC (Load resistance: Max 550 Ω) Output accuracy: Within $\pm 0.3\%$ of Transmission output 1 span 1-point Contact output: See 'Contact output (EVT option)'.
Transmission output 2 (TA2 option)	Converting pH or temperature to analog signal every input sampling period, outputs the value in current. (Factory default: Transmission output 1: Conductivity, Transmission output 2: Temperature) If Transmission output 2 high limit and low limit are set to the same value, Transmission output 2 will be fixed at 4 mA DC. Resolution: 12000 Current: 4 to 20 mA DC (Load resistance: Max 550 Ω) Output accuracy: Within $\pm 0.3\%$ of Transmission output 2 span

Dimensions
(Scale: mm)

Terminal
arrangement

1, 2: Conductivity sensor terminal (②-③)
A, B: Temperature compensation sensor terminals (⑤-⑥)
Pt100 (2-wire) or Pt1000
A, B, B: Temperature compensation sensor terminals (⑤-⑥-⑦)
Pt100 (3-wire)
E: Shield wire terminal (⑧)
POWER SUPPLY: Power terminals (⑬-⑭)
When EVT option is ordered:
A1: A1 output terminals (⑨-⑩)
A2: A2 output terminals (⑪-⑫)
When TA option is ordered:
A1: A1 output terminals (⑨-⑩)
TRANSMIT OUTPUT1: Transmission output 1 terminals (⑪-⑫)
When TA2 option is ordered:
TRANSMIT OUTPUT2: Transmission output 2 terminals (⑨-⑩)
TRANSMIT OUTPUT1: Transmission output 1 terminals (⑪-⑫)
RS-485: Serial communication modular jack
When no option is ordered, A1, A2, TRANSMIT OUTPUT1 and TRANSMIT OUTPUT2 terminals are not equipped.

Modular Jack Pin (WIL-102-ECL side arrangement)

Diagram illustrating the RS-485 connector pin assignments for two different configurations:

- Top Configuration:**
 - No. 1: COM
 - No. 6: NC
- Bottom Configuration:**
 - No. 1: YB(+)
 - No. 6: YA(-)